

Urea/Ammonia, UV method

Alternative Procedures Brochure

Introduction

This kit has been developed to work in cuvettes with a standard pathlength of 1 cm, as described in the respective "Product Brochure". However, it can be adapted for use in 96-well microplates or in auto-analysers (micro-volume formats) with minimal assay optimisation. Basically, the assay volumes for the cuvette format have to be reduced approximately 10-fold for use in microplate format or in auto-analyser format. However, when using these micro-volume formats, you must be aware that the radiation pathlength is usually smaller than the standard cuvette pathlength of 1 cm. Thus, to perform the calculation of the amount of analyte in the samples under analysis follow one of the three strategies described in the section below.

Strategies for analyte calculation

Auto-analysers use reaction volumes of approximately 0.315 ml and pathlengths from 4 to 8 mm, which is similar to a standard 96-well microplate in which the same reaction volume would have a pathlength of 6 or 7 mm (similar assay volumes). Therefore, in both formats (96-well microplate and auto-analysers systems), the calculation of the analyte must be done by one of the three possible methods described below:

1. Using the pathlength conversion factor

This is the easiest method to perform the calculation of the analyte. However, it requires a microplate reader with pathlength conversion capacity, i.e., the apparatus can detect the pathlength of each well and convert the individual

readings to a 1 cm pathlength (cuvette format). In the case of auto-analysers, the absorbance readings should be directly converted to a 1 cm pathlength. This will allow the calculation of the analyte content as described in the "Product Brochure", provided with the kit and available at the NZYTech website.

2. Using one standard curve

In this method, it is necessary to perform a standard curve of the analyte on each microplate that contains the test samples, or in the auto-analyser, and calculate the result from the standard curve of analyte concentration vs. absorbance. The standard curve can be performed by using the control solution provided in the kit.

3. Using two standard curves

The most complicated method is to perform standard curves of the analyte in both the cuvette format (i.e. with a 1 cm of radiation pathlength) and the 96-well microplate or auto-analyser formats, and use these results to obtain a mean conversion factor between the cuvette procedure values and the alternative procedure values. The standard curves can be performed by using the control solution provided in the kit.

Please enquire info@nzytech.com to obtain any additional information about this kit, including additional specific procedures and applications.

V1901

Urea/Ammonia, UV method

Catalogue number: AK00101, 50 tests of each

Alternative Procedures Brochure

Introduction

This kit has been developed to work in cuvettes with a standard pathlength of 1 cm, as described in the respective "Product Brochure". However, it can be adapted for use in 96-well microplates or in auto-analysers (micro-volume formats) with minimal assay optimisation. Basically, the assay volumes for the cuvette format have to be reduced approximately 10-fold for use in microplate format or in auto-analyser format. However, when using these micro-volume formats, you must be aware that the radiation pathlength is usually smaller than the standard cuvette pathlength of 1 cm. Thus, to perform the calculation of the amount of analyte in the samples under analysis follow one of the three strategies described in the section below.

Strategies for analyte calculation

Auto-analysers use reaction volumes of approximately 0.315 ml and pathlengths from 4 to 8 mm, which is similar to a standard 96-well microplate in which the same reaction volume would have a pathlength of 6 or 7 mm (similar assay volumes). Therefore, in both formats (96-well microplate and auto-analysers systems), the calculation of the analyte must be done by one of the three possible methods described below:

1. Using the pathlength conversion factor

This is the easiest method to perform the calculation of the analyte. However, it requires a microplate reader with pathlength conversion capacity, i.e., the apparatus can

detect the pathlength of each well and convert the individual readings to a 1 cm pathlength (cuvette format). In the case of auto-analysers, the absorbance readings should be directly converted to a 1 cm pathlength. This will allow the calculation of the analyte content as described in the "Product Brochure", provided with the kit and available at the NZYTech website.

2. Using one standard curve

In this method, it is necessary to perform a standard curve of the analyte on each microplate that contains the test samples, or in the auto-analyser, and calculate the result from the standard curve of analyte concentration vs. absorbance. The standard curve can be performed by using the control solution provided in the kit.

3. Using two standard curves

The most complicated method is to perform standard curves of the analyte in both the cuvette format (i.e. with a 1 cm of radiation pathlength) and the 96-well microplate or auto-analyser formats, and use these results to obtain a mean conversion factor between the cuvette procedure values and the alternative procedure values. The standard curves can be performed by using the control solution provided in the kit.

Please enquire info@nzytech.com to obtain any additional information about this kit, including additional specific procedures and applications.

AK0010_IFU_sup_EN_V2301

Urea/Ammonia, UV method

| | |
|-------------------------|---------------------|
| Catalogue number | Presentation |
| AK00101 | 50 tests of each |

Application


This rapid and simple specific enzymatic method is used for the simultaneous determination of urea and ammonia (ammonium ions) in foodstuffs such as wine, fruit juice, bakery products, dairy products, egg products, meat and seafood, as well as in paper, fertilizer, pharmaceuticals, cosmetics, water and biological samples.

Introduction

Urea is the most important product of protein metabolism in mammals and the most abundant organic compound in their urine. Ammonia is mainly produced by microbial protein catabolism of organic materials. Therefore, these analytes may be used as reliable quality indicators for food products such as fruit juice, milk, cheese, meat and seafood. Urea and/or ammonia may also be used as indicators of the presence of faeces, urine and microorganisms in water.

In the wine industry, ammonia determination is important in the calculation of yeast available nitrogen (YAN). This kit uses a glutamate dehydrogenase that is not inhibited by tannins found in grape juice and wine. However, YAN comprises three components: free ammonium ions, amino nitrogen from free amino acids and from the side chain of L-arginine. Thus, for the most accurate determination of YAN, all three components should be quantified, which is possible by using NZYtech's L-Arginine/Urea/Ammonia kit.

Principle

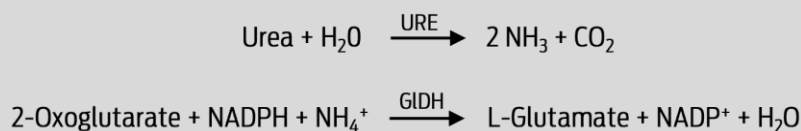

The amount of NADPH consumed through the combined action of urease and glutamate dehydrogenase (GIDH), measured at 340 nm, is stoichiometric with the amount of urea and ammonia in sample volume.

Specificity

The determination is specific for urea and ammonia.

Sensitivity and detection limit

The sensitivity of the assay is based on 0.005 absorbance units and a sample volume $v = 2.00$ mL. This corresponds to ammonia and urea concentrations of 0.018 and 0.031 mg/l sample solution, respectively, when measured at 340 nm. The detection limit of 0.07 and 0.13 mg/L for ammonia and urea, respectively, is derived from the absorbance difference of 0.020 (340 nm) and a maximum sample volume $v = 2.00$ mL.

Linearity and precision

Linearity of the determination exists from 0.2 μg to 7 μg ammonia/assay. Regarding urea, linearity of the determination is guaranteed from 0.3 μg to 14 μg urea/assay. In a double determination using one sample solution, a difference of 0.005 to 0.010 absorbance units may occur for ammonia (0.005 to 0.015 for urea). The relative standard deviation ("coefficient of variation") is approx. 1 to 2% for ammonia and 1 to 3% for urea.

Kit composition

Solution 1. TEA buffer (25 mL, 0.5 M, pH 8.0) plus imidazole (200 mM), 2-oxoglutarate (40 mM) and sodium azide (0.02 % w/v) as a preservative. Store at 2 °C to 8 °C.

Tablets 2. 150 tablets of NADPH supplied in a plastic vial containing desiccant. Allow this container to warm to room temperature (in the presence of a desiccant if possible) before opening to remove tablets. Store desiccated 2 °C to 8 °C (Long term storage: -30 °C to -15 °C)

Add 3 tablets and 0.5 mL of solution 1 per assay, including blank reaction, to a test tube and stir intermittently over 2-3 min (Solution 1+2).

Suspension 3. Glutamate dehydrogenase (GIDH) is provided in 2.5 M lithium sulphate (EC 1.4.1.2; 1.1 mL). Store at 2 °C to 8 °C. Swirl bottle before use.

Suspension 4. Urease is provided in 2.5 M lithium sulphate (EC 3.5.1.5; 1.1 mL). Store at 2 °C to 8 °C. Swirl bottle before use.

Powder 5. Urea control powder (~2 g). Store at 2 °C to 8 °C.

Accurately weigh approx. 70 mg of urea into a 1 L volumetric flask, fill to the mark with distilled water and mix thoroughly. Prepare fresh before use. This control solution is stable for ~3 months at -30 °C to -15 °C.

Solution 6. Ammonia standard solution (5 mL, 0.04 mg/mL) in 0.02% (w/v) sodium azide. Store at 2 °C to 8 °C. This standard should be used when there is doubt about the method accuracy.

Protocol (endpoint analysis)

Wavelength: 340 nm

Cuvette: 1 cm light path (glass or plastic)

Temperature: ~25 °C

Final volume: 2.62 mL (ammonia); 2.64 mL (urea)

Sample solution: 0.2 – 7 µg of ammonia or 0.3 – 14 µg of urea per cuvette (in 0.1 – 2.0 mL sample volume)

Read absorbances against air (without cuvette in the light path), or against water

| PIPETTE INTO CUVETTES (mL) | BLANK | SAMPLE |
|---|-------|--------|
| Distilled water | 2.10 | 2.00 |
| Sample | - | 0.10 |
| Solution 1+2 (NADPH/TEA buffer) | 0.50 | 0.50 |
| Mix, measure the absorbance of the solutions (A1) after ~2 min and start the reaction by addition of | | |
| Suspension 3 (GIDH) | 0.02 | 0.02 |
| Mix, measure the absorbance of the solutions (A2) at the end of the reaction (approx. 3 min)*. Then add | | |
| Suspension 4 (Urease) | 0.02 | 0.02 |
| Mix, measure the absorbance of the solutions (A3) at the end of the reaction (approx. 5 min)* | | |

Mixtures can be obtained with a plastic spatula or by gentle inversion after sealing with a cuvette cap or Parafilm®.

* if necessary, continue to read the absorbances at 1 min intervals until the reaction ends.

Calculation

Determine the absorbance difference for both blank and sample (A1-A2). Subtract the absorbance difference of the blank from the absorbance difference of the sample, thereby obtaining $\Delta A_{\text{Ammonia}}$. Determine the absorbance difference for both blank and sample (A2-A3). Subtract the absorbance difference of the blank from the absorbance difference of the sample, thereby obtaining ΔA_{Urea} .

The concentrations of ammonia (g/L) and urea (g/L), based on the ϵ of NADH at 340 nm ($6300 \text{ L} \times \text{mol}^{-1} \times \text{cm}^{-1}$), are calculated as follows:

$$C(\text{ammonia}) = 0.07082 \times \Delta A_{\text{ammonia}} \quad [\text{g/L}]$$

$$C(\text{urea}) = 0.1258 \times \Delta A_{\text{urea}} \quad [\text{g/L}]$$

If the sample has been diluted or a different sample volume was used during the reaction, the result must be multiplied by the corresponding dilution/concentration factor.

Alternative procedures (micro-volumes)

Although this kit has been developed to work in cuvettes, it can be easily adapted for use in 96-well microplates or in auto-analysers. Basically, the assay volumes for the cuvette format have to be reduced approximately 10-fold for use in microplate format or in auto-analyser format. However, when using these micro-volume formats, you must be aware that the radiation pathlength is usually smaller than 1 cm, which is the

standard cuvettes pathlength. Thus, to perform the calculation of the amount of analyte in the samples follow one of the three possible strategies described in the "Alternative Procedures", available on the NZYtech website.

Interferences

If the conversion of urea and ammonia has been completed within the time specified in the assay, it can be generally concluded that no interference has occurred. However, this can be further checked by adding urea (~7 µg in 0.1 mL) or ammonia (~4 µg in 0.1 mL) to the cuvette on completion of the reaction. A significant decrease in the absorbance should be observed. Interfering substances in the sample being analysed can be identified by including an internal standard. Although tannins in fruit juice can lead to the inhibition of some GIDH, the enzyme used in this kit does not have this limitation.

General information on sample preparation

The amount of ammonia and urea present in the cuvette should range between 0.2 and 7 µg, and 0.3 and 14 µg, respectively. Thus, if a sample volume of 0.10 mL is used the sample solution must be diluted to yield ammonia and urea concentrations between 2 and 70 mg/L, and 3 and 140 mg/L, respectively. However, the sample volume can range from 0.10 to 2.00 mL, by replacing water (ammonia and urea range from 0.10 to 70 mg/L and 1.50 to 140 mg/L, respectively).

To implement this assay use clear, slightly coloured and practically neutral liquid samples directly, or after dilution; filter turbid solutions; degas samples containing carbon dioxide (e.g. by filtration); adjust acid samples, which are used undiluted for the assay, to approx. pH 8 by adding 2 M NaOH; measure "coloured" samples (if necessary adjusted to approx. pH 8) against a sample blank; treat "strongly coloured" samples that are used undiluted or with a higher sample volume with 0.2 g PVPP/10 mL of sample; crush or homogenize solid or semi-solid samples, extract with water or dissolve; extract samples containing fat with hot water at 60 °C.

Examples of sample preparation

Determination of urea and ammonia in grape must and wine

The concentration of urea and ammonia in white and red grape juice/must and wine can be determined usually without any sample treatment, except filtration and dilution, if necessary. For red wine, it may be required to remove some of the colour by the addition of 0.2 g of PVPP per 10 mL of sample. Shake the tube vigorously for 5 min and filter through Whatman No. 1 filter paper. No dilution is usually required and a sample volume of 25-50 µL is generally satisfactory.

Determination of urea and ammonia in fruit juices

Adjust 25 mL of filtered sample to a pH of approx. 8 using 2 M NaOH. Quantitatively transfer the solution to a 50 mL volumetric flask and adjust to volume with distilled water. If the solution is highly coloured, it may be necessary to add 0.2 g of PVPP/10 mL of sample. Shake the tube vigorously for 5 min and then filter through Whatman No. 1 filter paper. No dilution is usually required and a sample volume of 0.1 mL is generally satisfactory.

Determination of urea and ammonia in meat

Weigh approx. 5 g of meat or meat product into a 100 mL bottle. Add 20 mL of 1 M perchloric acid and homogenise for 2 min. Transfer to a 40 mL beaker and adjust the pH to approx. 8.0 using 2 M KOH. Subsequently transfer to a 100 mL volumetric flask and adjust to the mark with distilled water. Store on ice for 20 min to allow the precipitation of potassium perchlorate and fat separation. Filter, discarding the first 3-5 mL, and use the clear filtrate for the assay. Usually, no further dilution is required and a sample volume of 0.5 mL is satisfactory.

References

Bergmeyer, H. U. & Beutler, H.-O. (1990). Ammonia. In Methods of Enzymatic Analysis (Bergmeyer, H. U., ed.), 3rd ed., Vol. VIII, pp. 454-461, VCH Publishers (UK) Ltd., Cambridge, UK.

Recommendations

A method with less interferences than chemical methods recommended/approved by the:

- German and Dutch food laws;
- Recommended by the Mitteleuropäische Brautechnische Analysenkommission (MEBAK) (Central European Commission for Brewing Technology).

Please enquire info@nzytech.com to obtain any additional information about this kit, including additional specific applications

For life science research only. Not for use in diagnostic procedures.